

FIG. 1

Fig. 2A

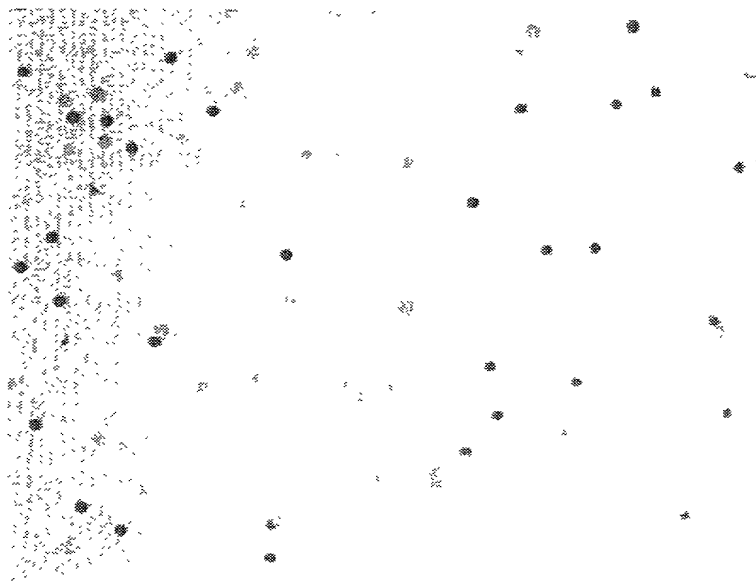


Fig. 2B

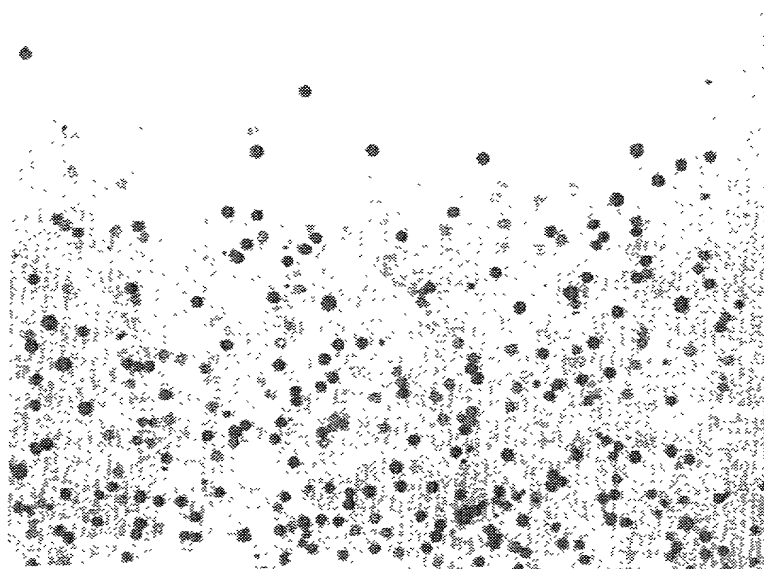


Fig. 3A

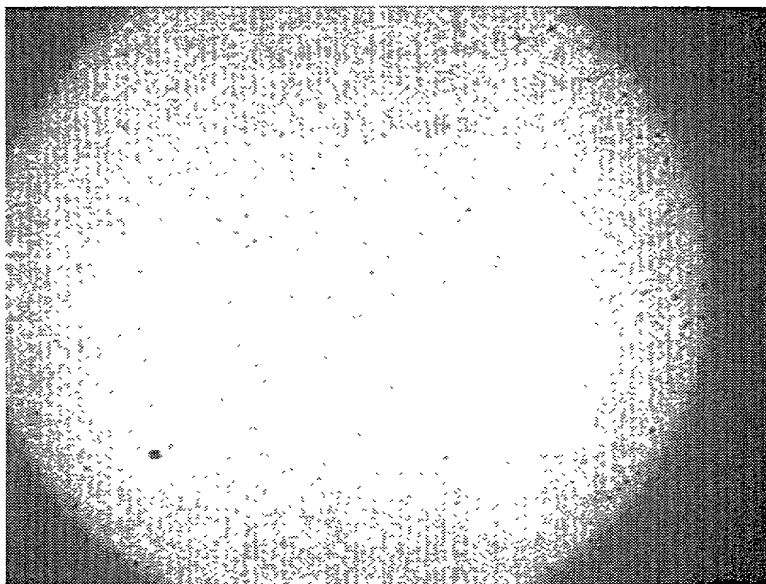
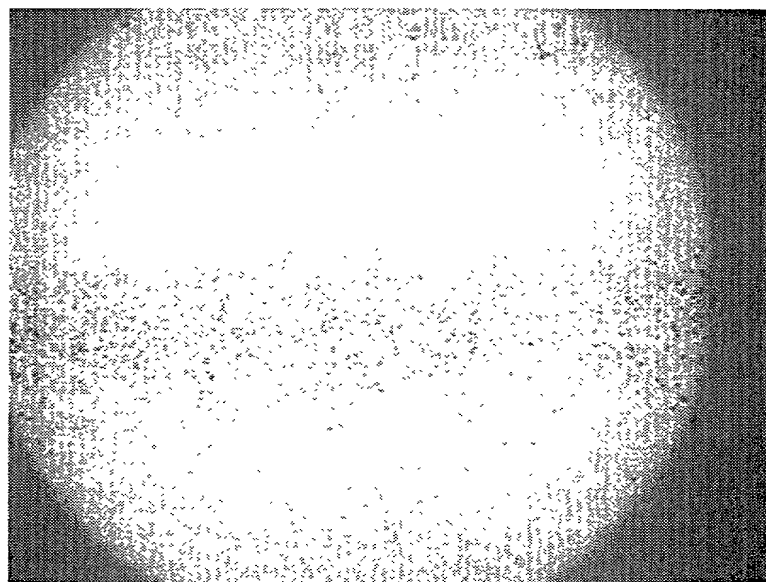


Fig. 3B



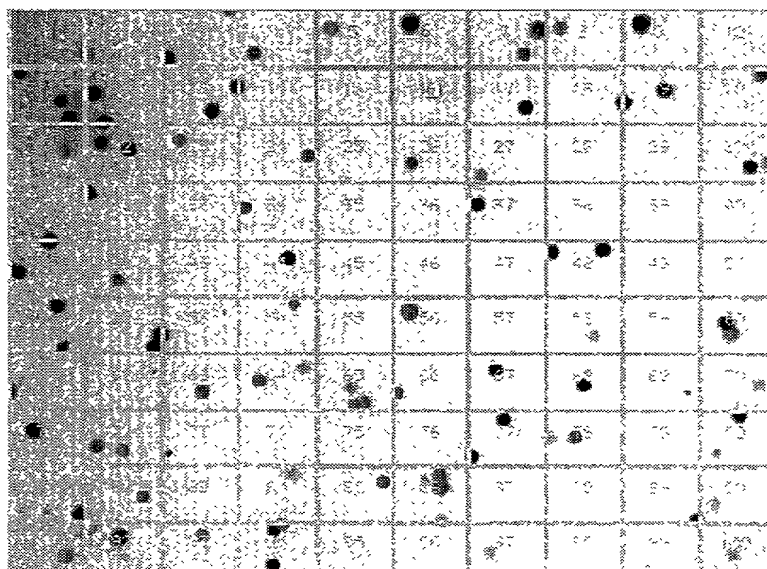


FIG. 4A

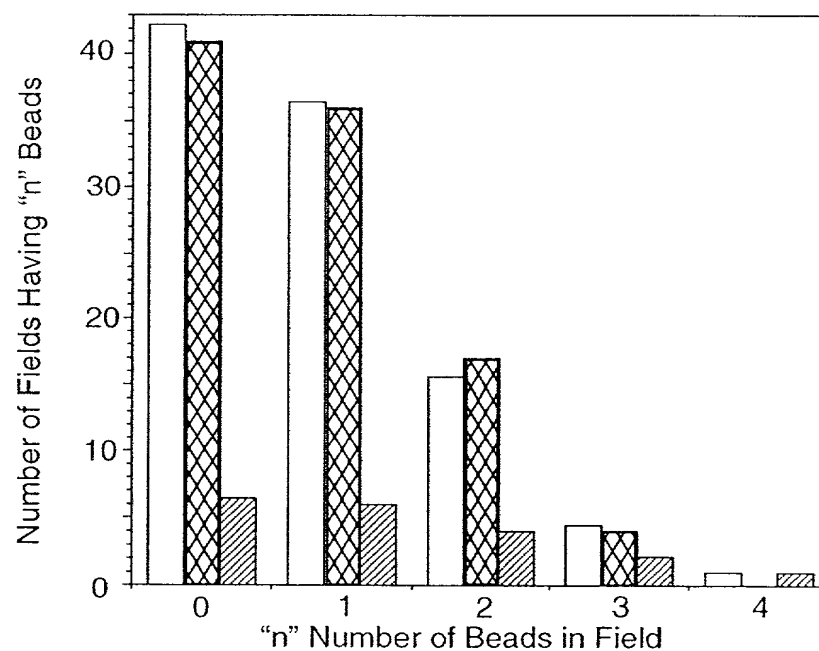


FIG. 4B

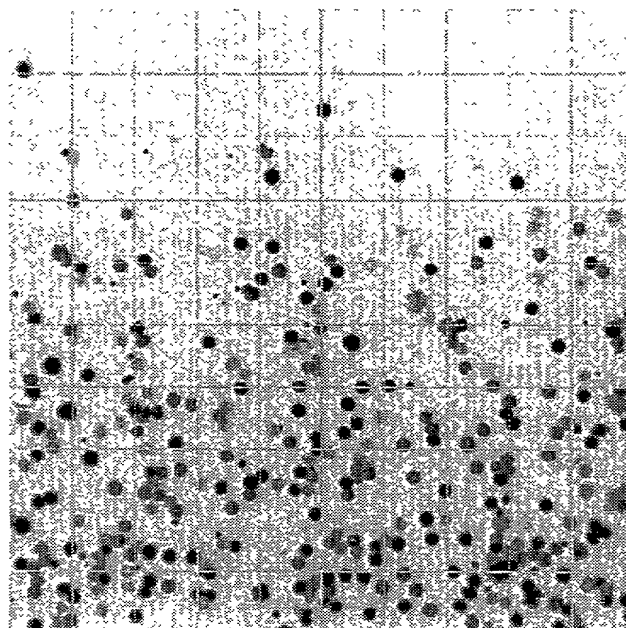


Fig. 5A

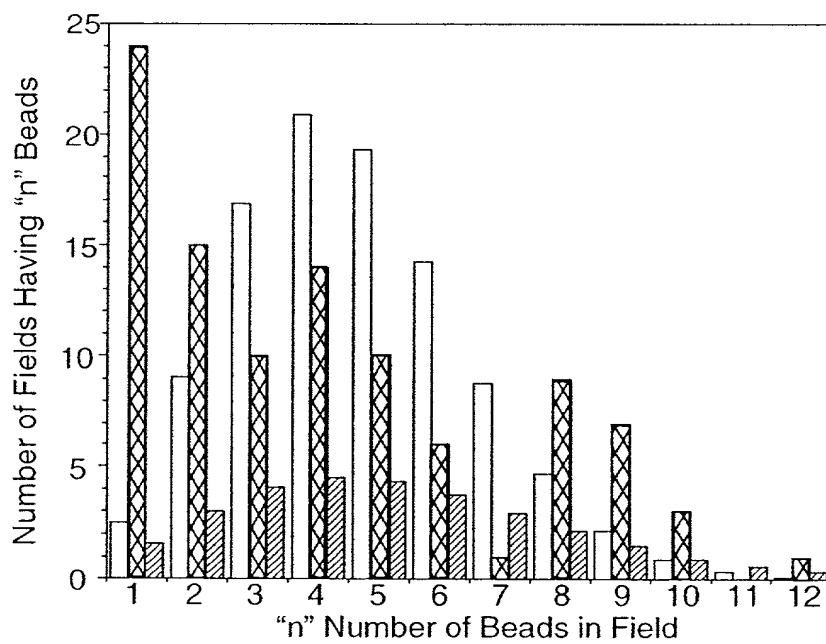


Fig. 5B

Description of Schematic

Diagram

- A. Color Beads DNA Microarray
- B. Illumination light source
- C. Cover Lid
- D. Light Deflector
- E. Lens
- F. Charge Coupled Device (CCD)
- G. Computer control unit

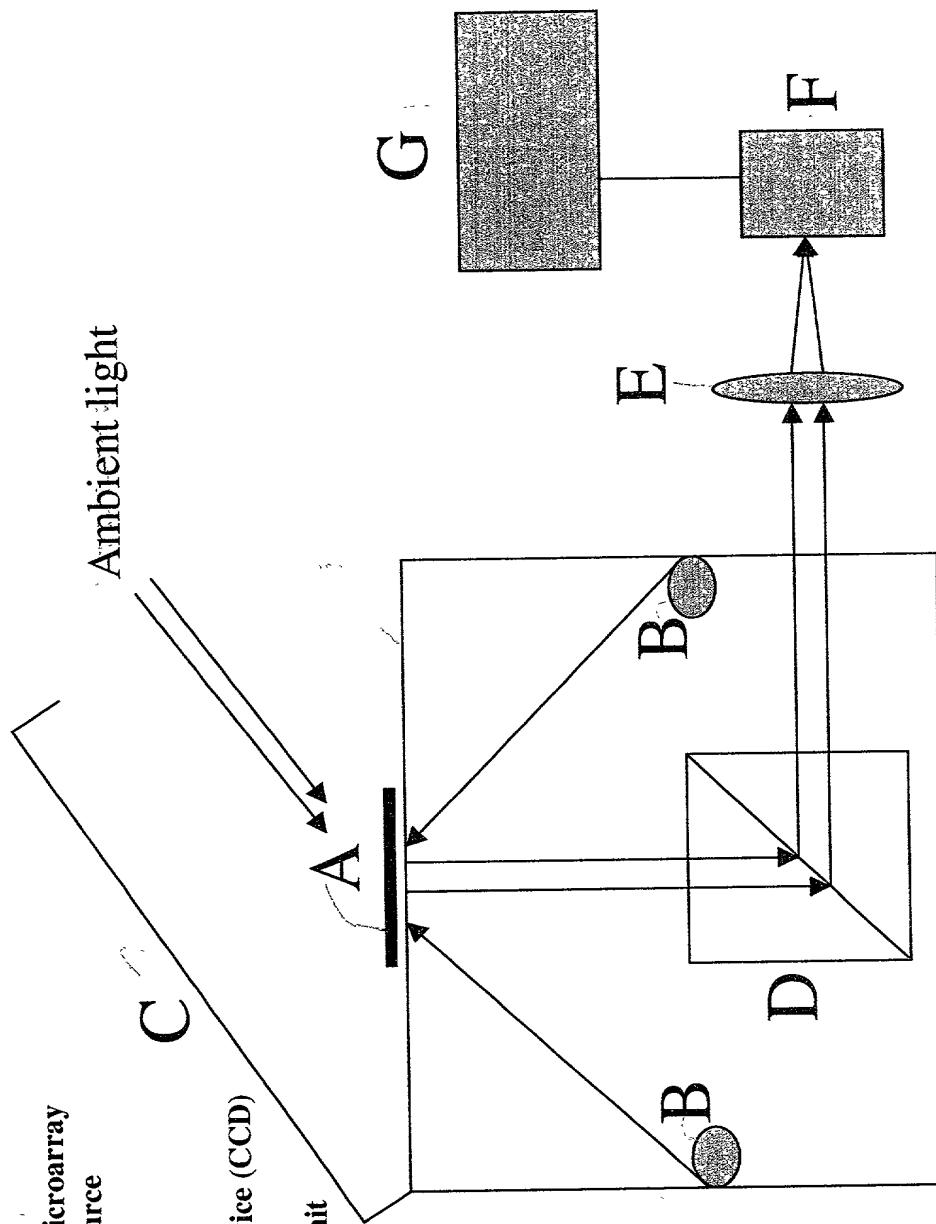


Fig. 7.

Workflow Chart of Nucleic Acid Random Microarray Analysis System

Step 1. Hybridization of chemiluminescently/fluorescently labeled nucleic acid sample onto the microsphere coated microarray



Step 2. Removal of non-specifically bound chemiluminescently/fluorescently labeled nucleic acid by washing the microarray in buffer solution



Step 3. Whole frame imaging capture of chemiluminescence/fluorescence image resulted from the hybridization interaction of unknown nucleic acid sequences with probe sequences (IMAGE1).



Step 4. Whole frame imaging capture of the microarray under bright field illumination to obtain microsphere color signature/barcode image (IMAGE2).



Step 5. Identification of unknown nucleic acid in the sample solution by computer analysis of IMAGE1 and IMAGE2 using pattern recognition algorithm.

100368220.122101

Fig 8 A

10036828-102101



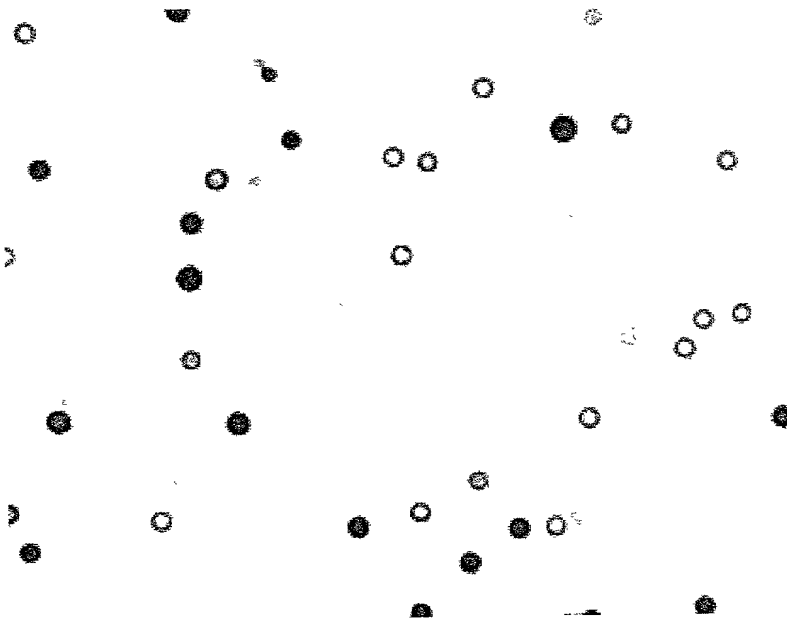


Fig 8 B

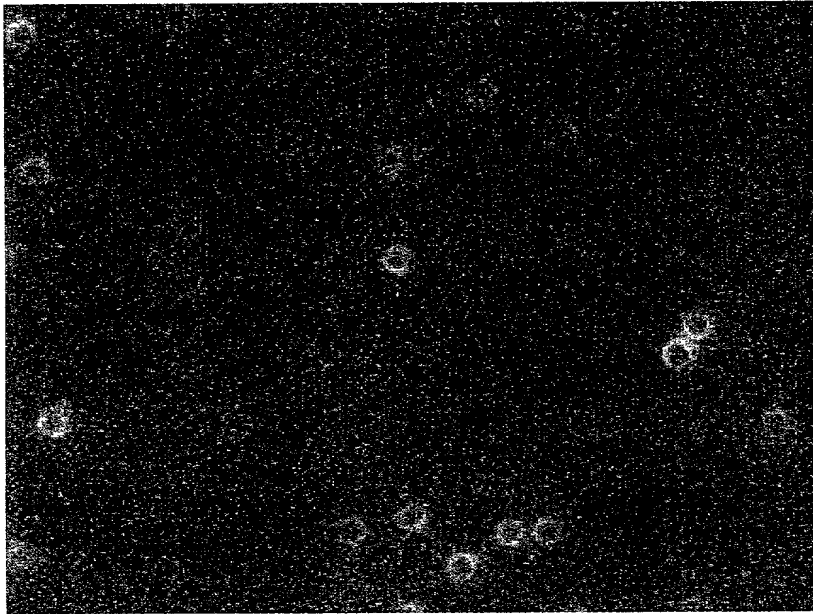


10036828 122104

Fig 9A

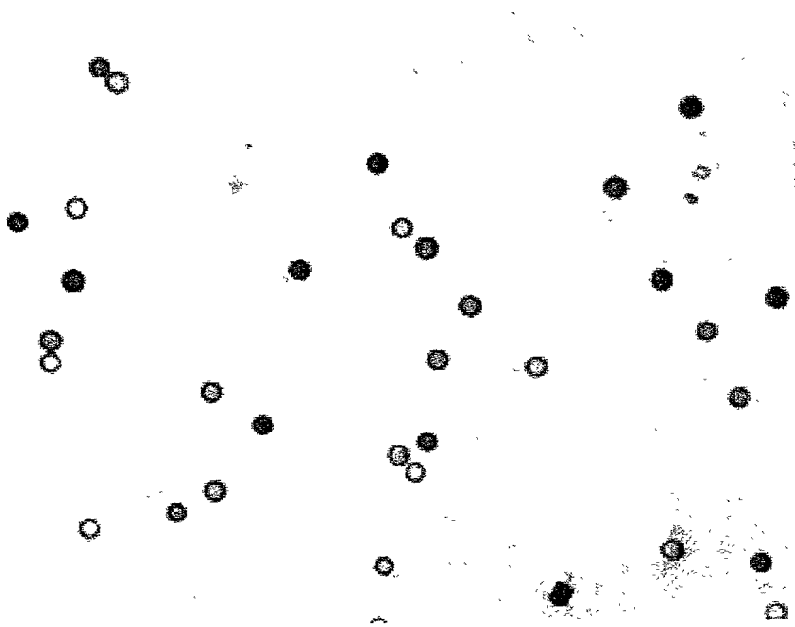

10036628.122101

Fig 9B

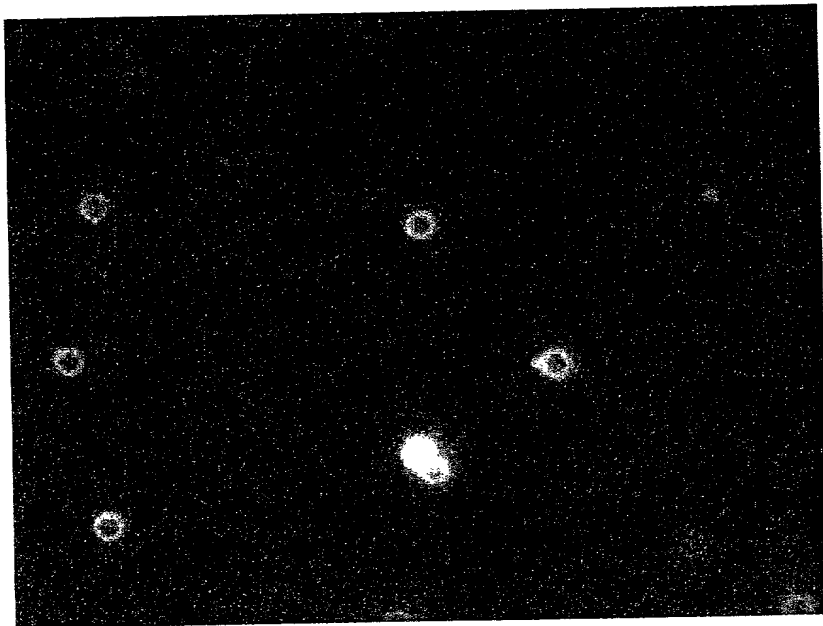

10036823 122101

10036828 102101

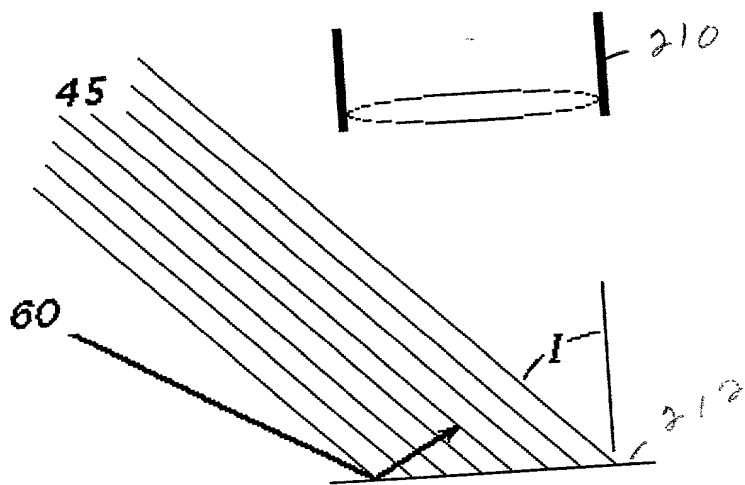


FIG. 10A

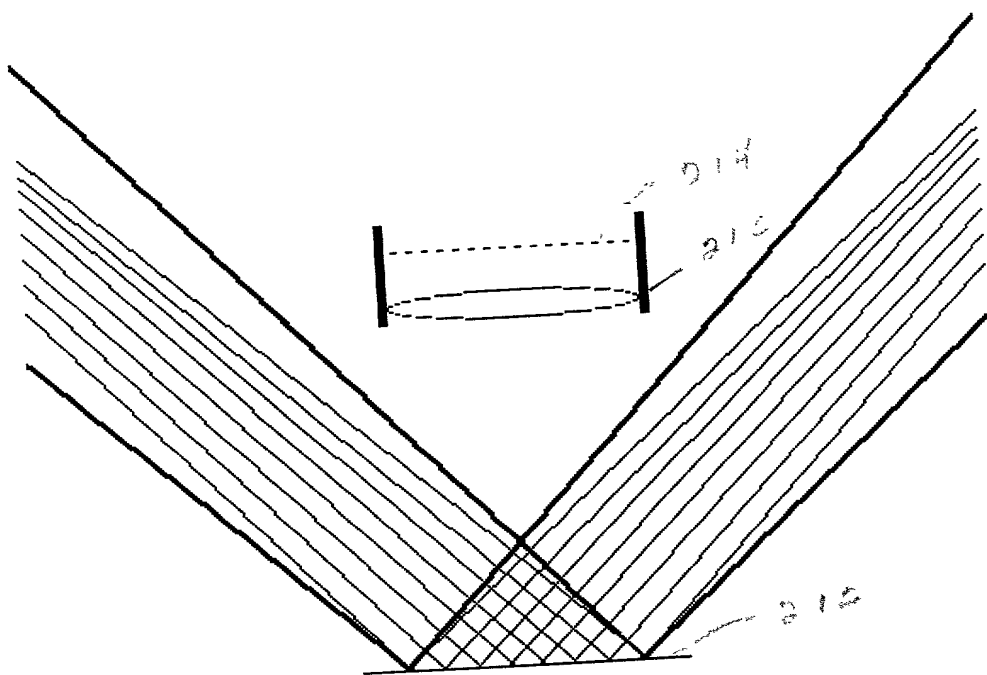


FIG. 10B

